

Fig. 1

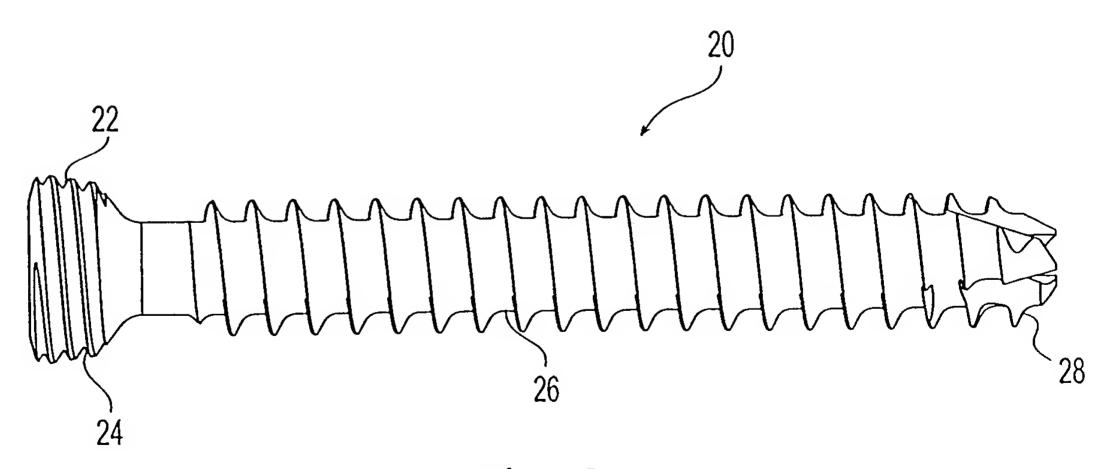


Fig. 2

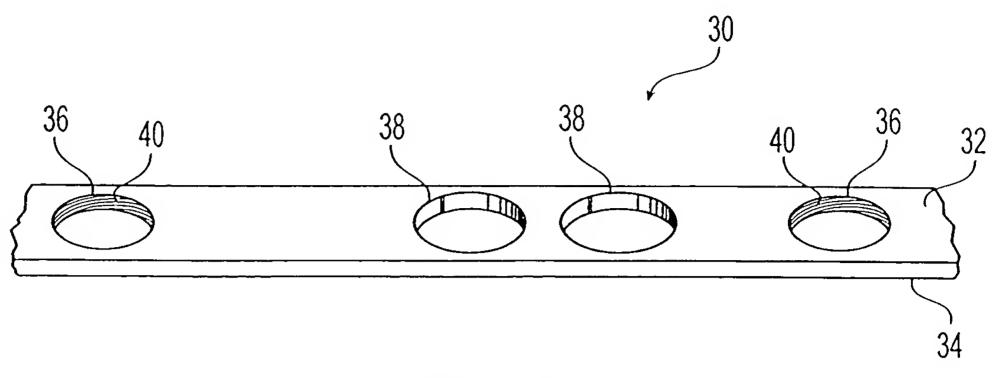


Fig. 3

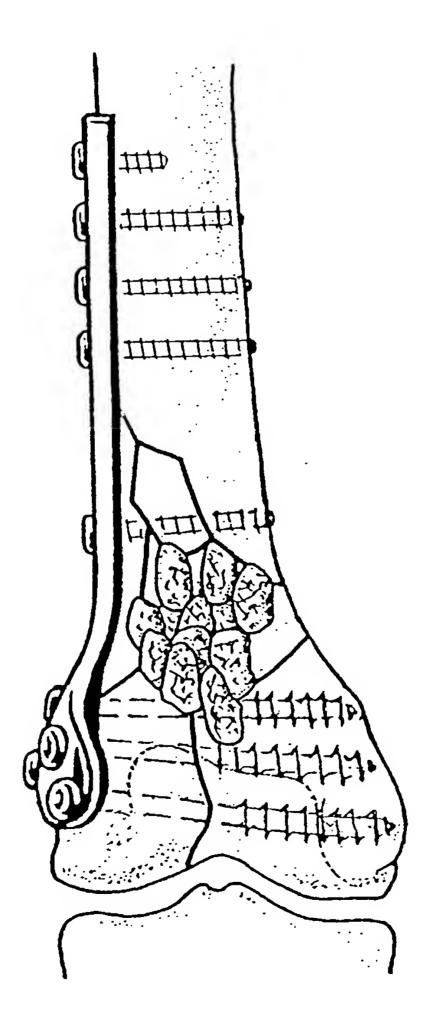


Fig. 9

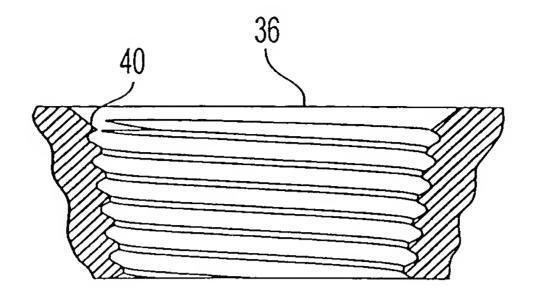


Fig. 4

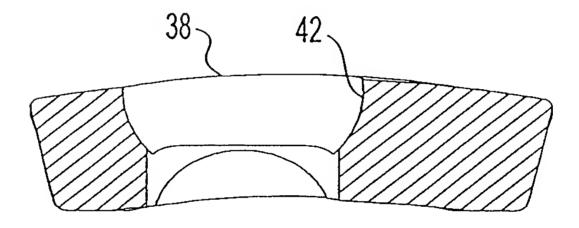


Fig. 5

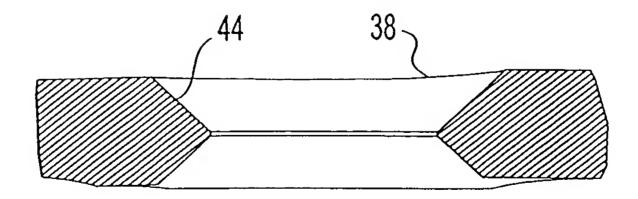
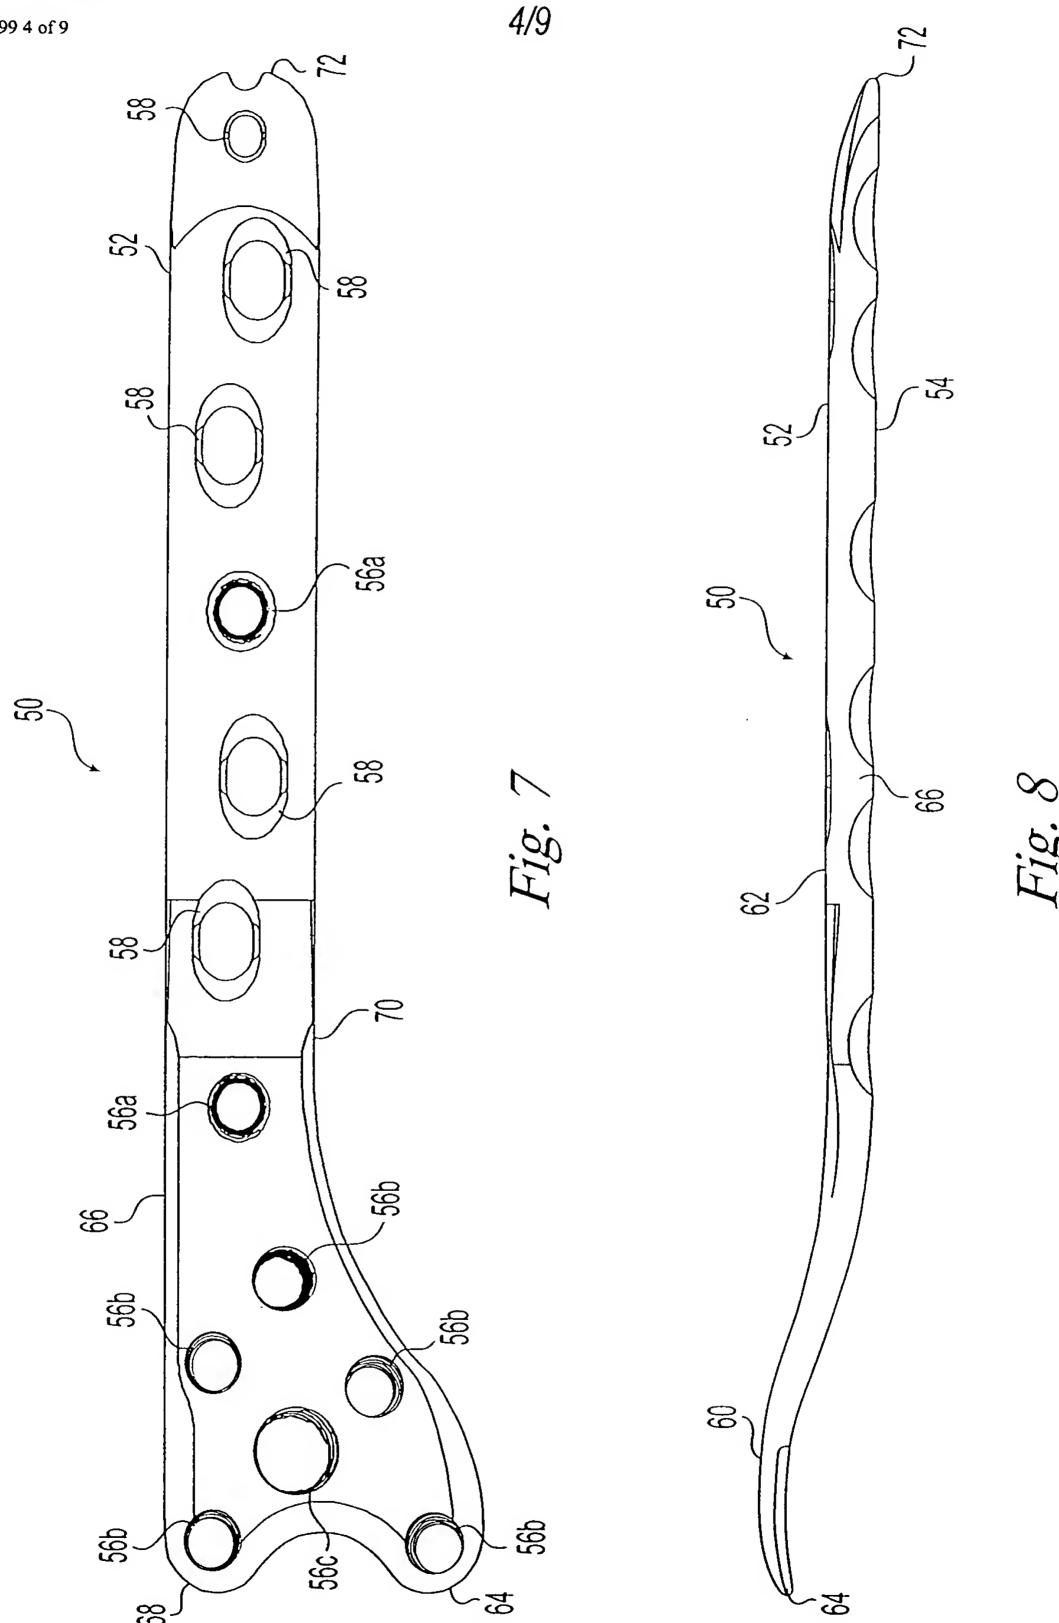
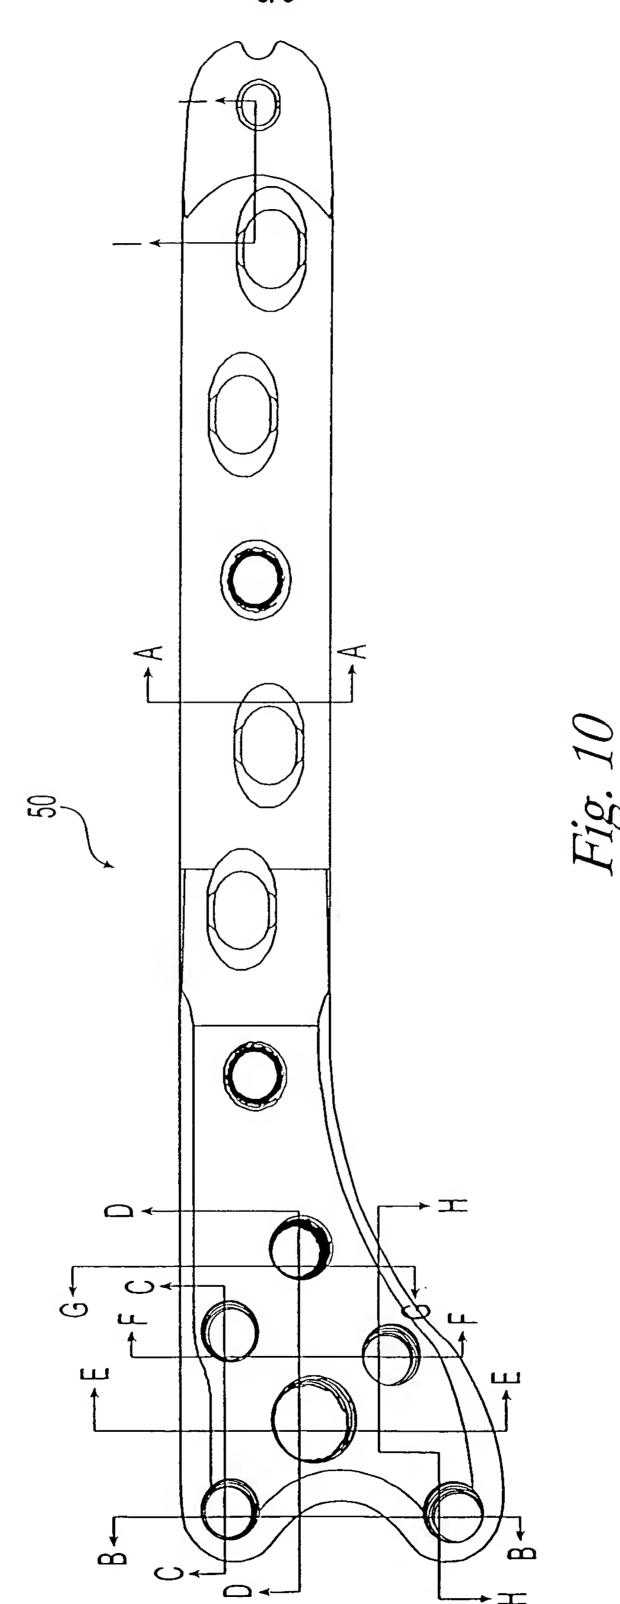


Fig. 6





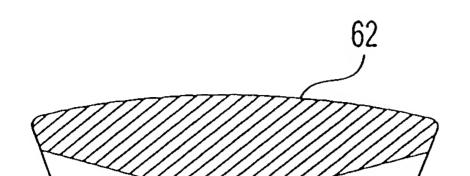
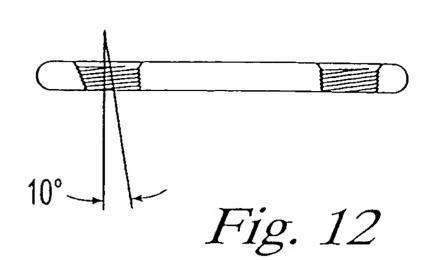


Fig. 11



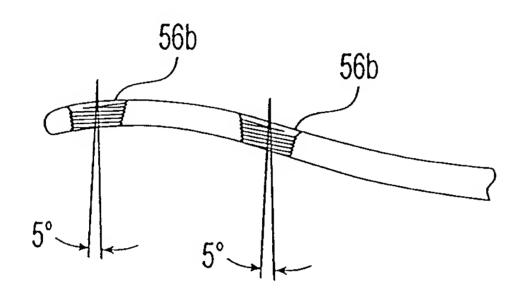


Fig. 13

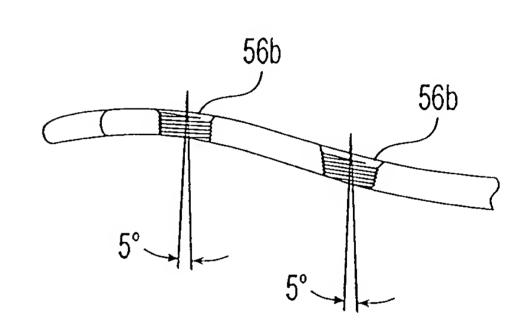


Fig. 14

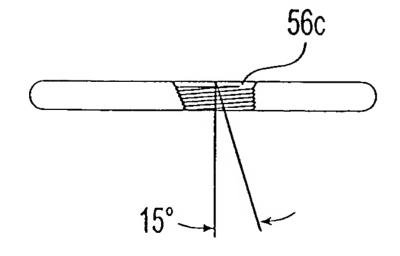


Fig. 15

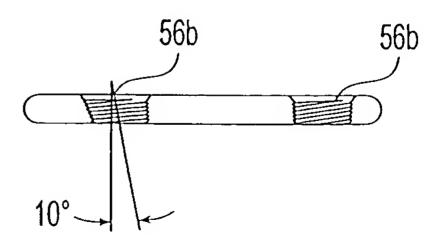


Fig. 16

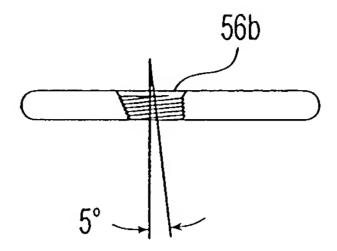


Fig. 17

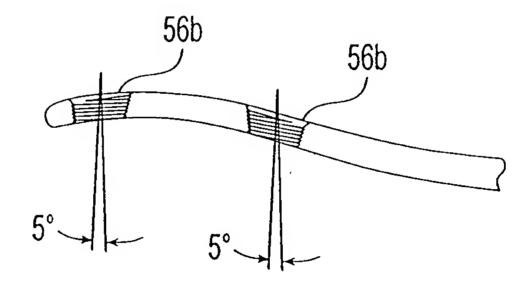


Fig. 18

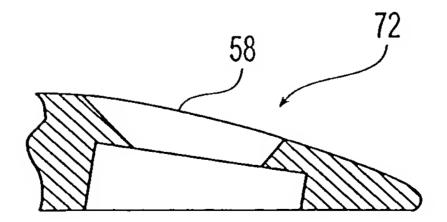


Fig. 19

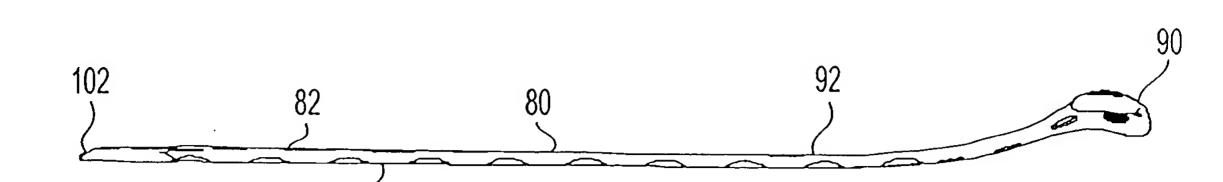
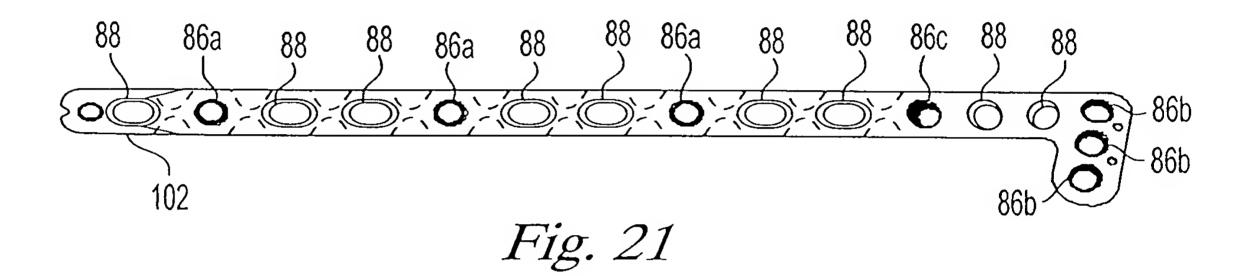


Fig. 20

84




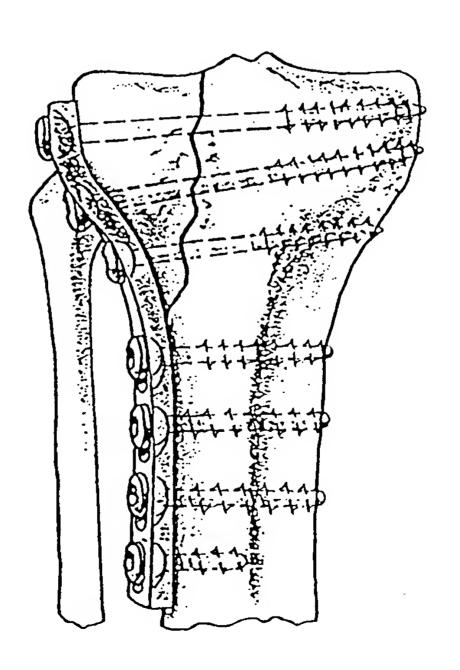


Fig. 22

Continuation of Patent Application of 09/660,287
Filed: Concurrently Herewith; By: WEAVER et al.
For: Bone Plating System; Pennie & Edmonds LLP (202)-496-4400 Atty Dkt. No. 8932-807-999 9 of 9



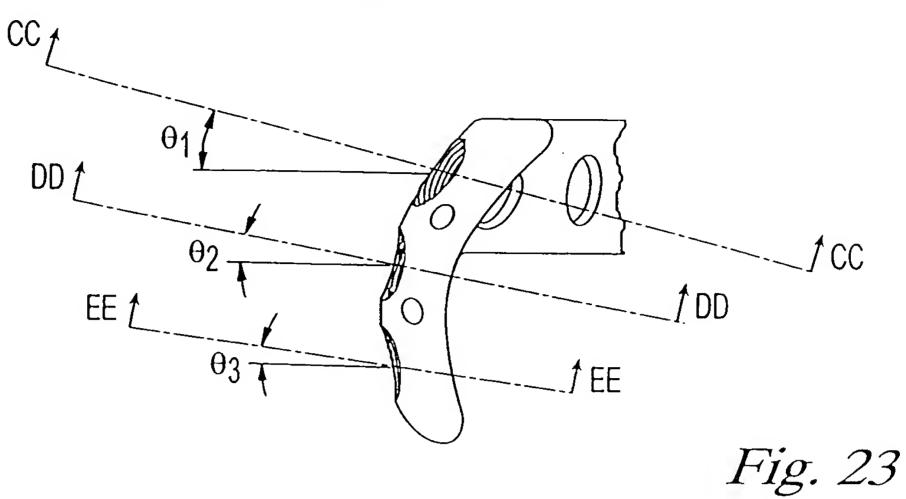

9/9




Fig. 24

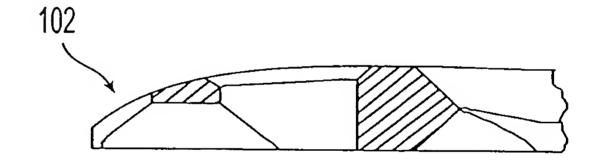


Fig. 25

